



**3-part differential
hematology analyzer
with ESR**

Integration


Transforming the possibility of IVD solutions

Infectious disease is spreading all over the world and becoming a serious problem. For example, 10 million people developed Tuberculosis (TB) which is one of the most serious infectious diseases, and TB caused an estimated 1.6 million deaths in 2017 according to data from the WHO.

What are your laboratory challenges?

What is required for a better clinical outcome?

Celltac $\alpha+$, equipped with ESR, can help to achieve a better clinical outcome.

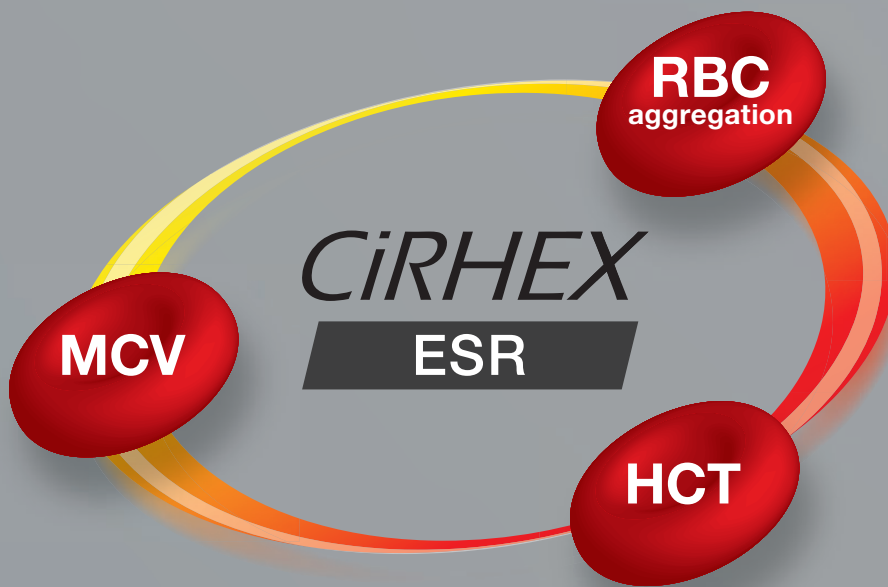

CiRHEX (Cell counter integrated rheometric excellence) technology can provide ESR result highly correlated with Westergren method by using HCT value and MCV value from CBC measurement and also RBC aggregation phenomenon.



Nihon Kohden's unique CiRHEX Technology helps you to achieve a better clinical outcome



Result displayed in 2 minutes by single EDTA tube for both CBC and ESR

A single EDTA tube can be used for both CBC and ESR measurement on our Celltac α+, and you will be able to get CBC results on the screen in 1 minute, and an ESR result in 2 minutes, with a single aspiration. This leads to reducing your workload, avoiding the risk of infection and providing a quick report to the patient.



Only 80 µL sample volume required for both CBC and ESR

Unlike the traditional methods for ESR testing, our Celltac α+ requires only 80 µL of blood sample for both CBC and ESR measurement. Not only does this small blood collection volume improve your laboratory workflow, it also improves the patient experience.



No additional reagents, no additional cost

As it is based on conventional hematology analyzers, diluent, detergent and hemolysing reagent are used for CBC and 3 part differential measurement on Celltac α+, but no additional reagents are required for ESR measurement.



Innovation


Maximizes laboratory productivity

Quality hematology testing



DynaHelix Flow technology perfectly aligns RBC and PLT cells for high impedance counting precision using an advanced hydrodynamic-focused sheath flow before passing through the aperture. In addition, the DynaHelix Flow totally prevents the risk of coincidence or re-entry of counted blood cells into the aperture, using the unique DynaHelix Flow stream.

This newly-developed advanced DynaHelix Flow Technology greatly improves counting precision and accuracy.

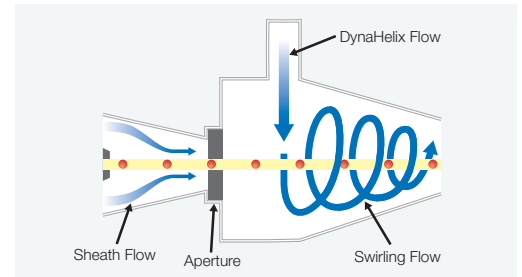

Integrated QC program



- QC program for ESR is available
- The same QC material can be used for CBC, 3 part diff and ESR
- QC lot management up to 25
- Assay value registration using a handy barcode reader (standard accessory)
- Automated judgement function (pass or fail)
- QC management by assay value, average value or Westgard multirule
- QC graph display and printout (optional)
- Automated calculation of statistical information such as average and SD

Reagent management



Photo: MEK-9100

Standard accessory, barcode reader



Celltac α+ reagent management system helps easier reagent bottle management with a unique barcode labeled on each reagent. Through this system and use of genuine Nihon Kohden reagents, testing quality is always maintained at a high level.

Thirty-one measuring parameters including ESR and other research parameters

Traditional CBC parameters, WBC 3 part differential parameters, Mentzer Index and RDWI, which are considered to be useful for Thalassemia screening. ESR and other parameters which are related to ESR are available on Celltac α+.

Operational excellence

Smart ColoRerun Assist helps to visually understand the reasons of re-measurement, by showing color-coded messages. This unique user-oriented function greatly improves workflow efficiency and maximizes productivity for faster test reports and clinical decision making.

YELLOW

A panic value (far outside the normal range) needs to be reported to a doctor immediately

ORANGE

Possibly incorrect data due to problems caused by the state of the blood sample or the measuring procedure

RED


Possibly incorrect data due to a technical problem with the instrument or measuring procedure



Sample ID	WBC	LY	10 ⁹ /L	Flag
Sample ID	WBC	LY	1.43	10 ⁹ /L
Patient ID	MD	0.04	(31.54)	WBC Panic Value
Date	GR	0.98	(65.79)	Leukopenia
Mode	RBC	4.65	10 ¹² /L	
	HCT	13.48	g/dL	
	HGB	41.3	g/L	
	MCV	88.8	fL	
	MCH	29.0	pg	
	MCHC	32.6	g/dL	
	RDW-CV	15.5	%	
	RDW-SD	44.4	fL	
	PLT	210.7	10 ⁹ /L	
	PCT	0.19	%	
	MPV	8.4	fL	
	PDW	16.1	%	
	P-LCR	44.0	%	



Sample ID	WBC	LY	10 ⁹ /L	Flag
Sample ID	WBC	LY	7.98	10 ⁹ /L
Patient ID	MD	0.20	(2.67)	
Date	GR	4.66	(65.79)	
Mode	RBC	6.22	H 10 ¹² /L	
	HCT	16.99	g/dL	
	HGB	52.0	g/L	
	MCV	89.6	fL	
	MCH	27.3	pg	
	MCHC	32.7	g/dL	
	RDW-CV	12.5	%	
	RDW-SD	44.4	fL	
	PLT	210.7	10 ⁹ /L	
	PCT	0.18	%	
	MPV	8.4	fL	
	PDW	16.1	%	
	P-LCR	44.0	%	

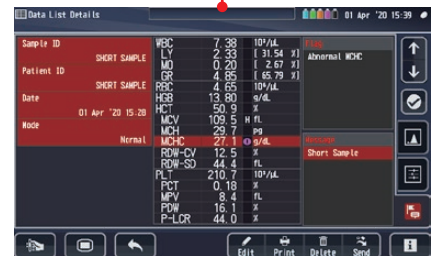

Sample ID	WBC	LY	10 ⁹ /L	Flag
Sample ID	WBC	LY	7.98	10 ⁹ /L
Patient ID	MD	0.20	(2.67)	
Date	GR	4.66	(65.79)	
Mode	RBC	6.22	H 10 ¹² /L	
	HCT	16.99	g/dL	
	HGB	50.9	g/L	
	MCV	109.5	H fL	
	MCH	29.7	pg	
	MCHC	27.1	g/dL	Abnormal MCHC
	RDW-CV	12.5	%	
	RDW-SD	44.4	fL	
	PLT	210.7	10 ⁹ /L	
	PCT	0.18	%	
	MPV	8.4	fL	
	PDW	16.1	%	
	P-LCR	44.0	%	

Seamless information transfer



Seamless Information Transfer

Celltac α+ supports seamless data transfer* to laboratory information systems through the LAN port or RS-232C port.

* ASTM protocol is available

Sister product

Celltac α MEK-1301/1302

Innovative hematology platform offering

- High quality CBC measurement based on DynaHelix Flow technology
- Smart ColoRerun Assist visually showing the reasons of re-measurement
- 23 measuring parameters including WBC 3 part differential
- Up to 60 samples/hour throughput (open mode)
- Complete QC program for laboratory accreditation requirements



MEK-1301
(open mode only)



MEK-1302
(open and closed mode)

Celltac α + MEK-1305

Key Specifications

- **Number of measuring parameters:** 31
WBC, LY%, MO%, GR%, LY#, MO#, GR#, RBC, HGB, HCT, MCV, MCH, MCHC, RDW-CV, RDW-SD, PLT, PCT, MPV, PDW, P-LCR, P-LOC, Mentzer Index*, RDWI*, ESR, ESR HCT Corr.* ESR TEMP Corr.*, SA*, AMP*, AI*, MIN*, t1/2*

* Research parameters

- **Measuring mode:** Open mode

Throughput

CBC + WBC 3 part differential: Approx. 60 samples/h
CBC + WBC 3 part differential + ESR: Approx. 20 samples/h

Sample volume

Normal mode: CBC + WBC 3 part differential 20 μ L
: CBC + WBC 3 part differential + ESR 80 μ L
Predilution mode: CBC 10 or 20 μ L
Capillary mode: CBC

Measuring method

WBC, RBC and PLT count- Electric impedance method
(DynaHelix Flow technology)
HGB: Colorimetric method
HCT: Calculated from RBC histogram
WBC differential: Calculated from WBC histogram
ESR: Calculated from sylectogram, HCT and MCV

Measuring range

WBC: 0.00 - 99.99 x 10³/ μ L, 0.00 - 299.90 x 10³/ μ L (High dilution mode)
RBC: 0.00 - 9.99 x 10⁶/ μ L
HGB: 0.00 - 29.90 g/dL
HCT: 0.0 - 99.9%
MCV: 20.0 - 199.0 fL
MCH: 10.0 - 50.0 pg
MCHC: 10.0 - 50.0 pg
PLT: 0.0 - 1490.0 x 10³/ μ L
ESR: 0 - 200 mm

- **Data storage capacity:** 50,000 data including histograms in the memory of the analyzer

Reproducibility and Linearity

Reproducibility

WBC: 2.0% or less (WBC: 4.00 x 10³/ μ L or more)
RBC: 1.5% or less (RBC: 4.00 x 10⁶/ μ L or more)
HGB: 1.5% or less
HCT: 1.5% or less
MCV: 1.0% or less
MCH: 2.0% or less
MCHC: 2.0% or less
PLT: 4.0% or less (PLT: 100.0 x 10³/ μ L or more)
ESR: 10.0% or less, or SD 1.5 mm or less

Linearity

WBC: Within \pm 3.00% or \pm 0.30 x 10³/ μ L (WBC: 0.20 to 99.9 x 10³/ μ L)
RBC: Within \pm 3.00% or \pm 0.08 x 10⁶/ μ L (RBC: 0.02 to 8.00 x 10⁶/ μ L)
HGB: Within \pm 1.50% or \pm 0.20 g/dL (HGB: 0.10 to 25.0 g/dL)
HCT: Within \pm 3.0% or \pm 1.0% (HCT: 20.0 to 60.0%)
PLT: Within \pm 10.0% or \pm 20.0 x 10³/ μ L (PLT: 10.0 to 1490.0 x 10³/ μ L)
(specifications above apply to normal mode)

Physical Specifications

- **Dimensions:** 230 W x 450 D x 428 H mm
- **Weight:** 21 kg
- **Line voltage:** 100 V to 240 V
- **Line frequency:** 50 or 60 Hz
- **Power input:** 150 VA
- **External output:** LAN x 1, USB x 2, RS-232C x 3

Environmental Conditions

- **Operating temperature:** 15 to 30°C
- **Operating humidity:** 30 to 85%
- **Operating atmospheric pressure:** 700 to 1060 hPa

Reagent

- **Diluent:** Isotonac 3 or Isotonac 4
- **Hemolysing reagent:** Hemolynac 310
- **Detergent:** Cleanac 710, Cleanac 3

IBSCGmedical
37 rue des Mathurins - 75008 Paris
Tél.+33 1 82 28 19 54

 direction.mc@ibscgmedical.net

