



Sample ID: 234567890123456789 | Patient ID: 98765432109876543210 | Patient Name: test_name_patient | Test Date: 2015/09/10 20:19

Parameter	Value	Unit	Reference Range
WBC	75.7	$10^9/\mu\text{L}$	
RBC	461	$10^{12}/\mu\text{L}$	
HGB	13.37	g/dL	
HCT	44.7	%	
MCH	97.0	pg	
MCHC	29.0	g/dL	
RDW-CV	29.9	L	
RDW-SD	16.2	H %	
PLT	66.8	$10^9/\mu\text{L}$	
PCT	20.11	L	
MPV	0.14	fL	
PDW	6.8	L %	
P-LCR	16.0	%	
NE	25.1	%	
LY	45.6	%	
MO	19.3	%	(60.29 %)
EO	7.1	%	(25.49 %)
BA	1.8	%	(9.42 %)
	1.9	%	(2.35 %)
			(2.45 H %)

Features :

Simultaneous 33 parameter measurement
 Micro sampling capability
 Status indicator
 Walk away autoloader
 Homogeneous built-in tube mixing
 STAT/tube by tube sample analysis
 DynaHelix Flow technology
 DynaScatter Laser technology
 Smart ColoRac Match
 Integrated validation station with touch screen
 Reagent and controls bardoce management
 Color 10.4-inch LCD touch screen
 3 different dilution measurements
 Automatic self-check, priming and nozzle cleaning
 Complete QC programs : L & J / Westgard Multi rule /
 \bar{X} B(\bar{X} Batch) management
 Access restriction with password
 Connection capability : RS232 / USB (Handy barcode, printer) /
 Handy barcode reader / Printer / LAN / HL7

Physical Specifications :

Dimensions and Weight :
 Dimensions : 675 W x 589 D x 576 H mm
 Weight : approx. 66 kg
 Power Requirements :
 • Line voltage : AC 100 to 240 V \pm 10% AC, 50/60 Hz
 • Power input : max 330 VA
 Sound Pressure Level : < 85dB
 Parameters :
 WBC, RBC, HGB, HCT, MCV, MCH, MCHC, RDW-CV, RDW-SD,
 PLT, PCT, MPV, PDW, P-LCR, NE, NE%, LY, LY%, MO, MO%, EO,
 EO%, BA, BA%, P-LCC*, Mentzer Index*, RDWI*, IG%*, IG#*,
 Band%*, Band#*, Seg%*, Seg#*
 (*) RUO parameters (Research Use Only)
 Throughput :
 • Auto and manual measurement up to 90 samples/hour
 Patient memory capacity : 10,000 patient with graphs
 Sample Volume : • CBC : 25 μ L
 • CBC+DIFF : 40 μ L
 • Pre-dilution mode : 20 μ L
 Barcode Format :
 Acceptable formats with or without check digits :
 Industrial 2 of 5, ITF, JAN/EAN/UPC, NW-7, CODE 39,
 CODE 93, CODE 128

Methods and Technologies :

- WBC, RBC, PLT : Electrical resistance (DynaHelix Flow technology)
- HGB : Colorimetric method (surfactant method)
- HCT : Calculated from RBC histogram
- WBC differentiation : Light scatter by laser (DynaScatter Laser technology)
- MCV, MCH, MCHC : Calculated from RBC, HGB and HCT
- PCT : Calculated from PLT histogram
- MPV : Calculated from PLT and PCT
- RDW-CV, RDW-SD : Calculated from RBC histogram
- PDW and P-LCR : Calculated from PLT histogram
- WBC population : Calculated from scattergram

Linearity and Reproducibility :

Precision (Reproducibility)
 WBC : 2.0% or less (WBC : $4.00 \times 10^3/\mu$ L or more)
 RBC : 1.5% or less (RBC : $4.00 \times 10^6/\mu$ L or more)
 HGB : 1.5% or less
 HCT : 1.5% or less
 MCV : 1.0% or less
 PLT : 4.0% or less (PLT : $100 \times 10^3/\mu$ L or more)
 NE% : 5.0% or less (NE% : 30.0% or more AND WBC : $4.00 \times 10^3/\mu$ L or more)
 LY% : 5.0% or less (LY% : 15.0% or more AND WBC : $4.00 \times 10^3/\mu$ L or more)
 MO% : 12.0% or less (MO% : 5.0% or more AND WBC : $4.00 \times 10^3/\mu$ L or more)
 EO% : 20.0% or less OR within ± 1.0 EO% (WBC : $4.00 \times 10^3/\mu$ L or more)
 BA% : 30.0% or less OR within ± 1.0 BA% (WBC : $4.00 \times 10^3/\mu$ L or more)
 NE : 8.0% or less (NE : $1.20 \times 10^3/\mu$ L or more)
 LY : 8.0% or less (LY : $0.60 \times 10^3/\mu$ L or more)
 MO : 20.0% or less (MO : $0.20 \times 10^3/\mu$ L or more)
 EO : 25.0% or less OR within $\pm 0.10 \times 10^3/\mu$ L (WBC : $4.00 \times 10^3/\mu$ L or more)
 BA : 30.0% or less OR within $\pm 0.10 \times 10^3/\mu$ L (WBC : $4.00 \times 10^3/\mu$ L or more)
 (Specifications above applies to normal mode)

Linearity

- WBC : within $\pm 3.0\%$ OR $\pm 0.3 \times 10^3/\mu$ L (WBC : 0.20 to $99.9 \times 10^3/\mu$ L)
 - RBC : within $\pm 3.0\%$ OR $\pm 0.08 \times 10^6/\mu$ L (RBC : 0.02 to $8.00 \times 10^6/\mu$ L)
 - HGB : within $\pm 1.5\%$ OR ± 0.2 g/dL (HGB : 0.10 to 25.0 g/dL)
 - HCT : within $\pm 3.0\%$ OR $\pm 1.0\%$ (HCT : 20.0 to 60.0%)
 - PLT : within $\pm 10.0\%$ OR $\pm 20 \times 10^3/\mu$ L (PLT : 10 to $1490 \times 10^3/\mu$ L)
- (Specifications above applies to normal mode)

Safety Standards Certification :

- IEC 60825-1 : 2014
- IEC 61010-1 : 2001
- IEC 61010-2-101 : 2002
- IEC 61326-2-6 : 2005
- EN 55011 : 2002 Group 1 Class B
- EN 60825-1 : 2014
- EN 61010-2-101 : 2002
- EN 61326-2-6 : 2006

EMC Standards :

- IEC 61326-2-6 : 2005
- EN 55011 : 2002 Group 1 Class B
- EN 61326-2-6 : 2006

Environmental Conditions :

- Operating temperature : 15 to 30°C (59 to 86°F)
- Operating humidity : 30 to 85%
- Operating atmospheric pressure : 700 to 1060 hPa


SARL au Capital de 7000 - Siège social : 37 rue des Mathurins 75008 PARIS

RCS Paris 789196417 - APE 7490B - Tel : + 33 1 82 28 19 54

Dépôt : 15 rue de la Garenne 27950 Saint-Marcel - Tel : + 33 2 32 54 04 26 - Fax : + 33 1 82 28 19 55

Smart ColoRac Match

Celltac G Smart ColoRac Match helps fast and easy location of clinically abnormal tubes as well as scan-failed barcoded tubes using the unique color-coded rack system that is associated with data management software on the analyzer. This unique user-oriented Smart ColoRac Match system enhances lab's efficiency without extra investment, extra space and special operator training. The Smart ColoRac Match surely maximizes lab's productivity for faster and more accurate test report.

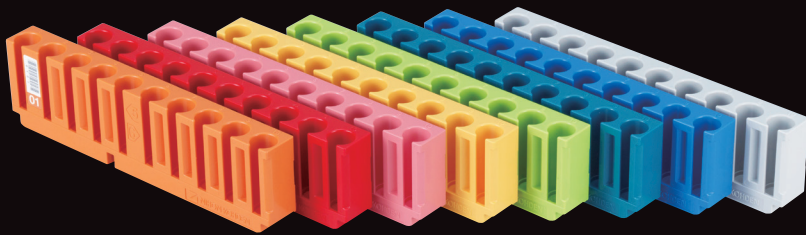

Data List		John Smith		2015/09/15 19:00:33								
Rack		Measurement Unit Ready										
Sample ID	Patient ID	Patient Name	Test Date	P/E	Check	A/M	Rack					
01234567890123456789	98765432109876543210	test_name.patient	2015/09/10 20:09	E		A	0503					
All	Finished Rack	1	2	3	4	5	6	7	8	9	10	
	Rack 06	○	○	○	○	○	○	○	○	○	○	○
	Rack 05	○	P	E	○	○	○	○	○	○	○	○
	Rack 04	○	○	○	○	○	○	○	○	○	○	○
	Rack 03	○	○	○	○	○	○	○	○	○	○	○
	Rack 02	○	○	○	○	○	○	○	○	○	○	○
	Rack 01	○	○	○	○	○	○	○	○	○	○	○

- P : There are some items determined as positive
- E : Measurement error
- B : Barcode error



Transforming the possibility of IVD solutions



Complete hematology platform offering:

- Up to 90 samples per hour
- 33 parameters
- Micro sampling capability
- Continuous loading of samples via rack fed system up to 7 racks of 10 tubes
- STAT/manual sample analysis
- Laser scatter + flow cytometry technology
- Built-in rocking mixing
- Smart ColoRac Match system
- Integrated validation station with touch screen
- Reagent and controls management with barcode

Status indicator




Celltac G status indicator is located in the front panel and clearly illustrates different operating status of the analyzer. For example, the operator can quickly recognize the need for reagent replacement by just looking at the status indicator turning red.

Homogeneous tube mixing



Each tube is picked up one by one from color-coded racks and gently mixed with built-in complete tube inversion mixing arm. Our auto-loading system contributes to faster test report to clinical decision makers and enhances workflow efficiency.


STAT mode

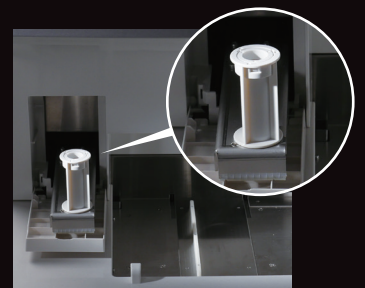

STAT and Pre-dilution modes analyze micro-samples such as pediatric blood collected from the earlobe or fingertip. Celltac G provides solutions based on the true laboratory needs.


Innovation for superior reliability

DynaHelix Flow

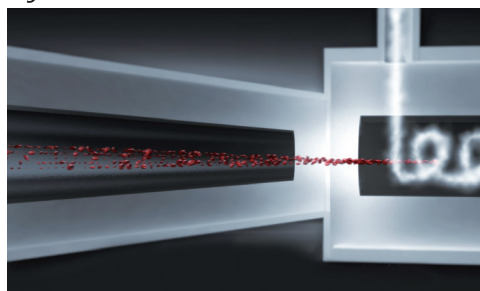

The DynaHelix Flow technology perfectly aligns WBC, RBC and PLT cells for high impedance counting precision using advanced hydrodynamic-focused sheath flow before passing through the aperture. In addition, the DynaHelix Flow totally prevent risk of coincidence or count of blood cell re-entry into the aperture using unique DynaHelix Flow stream. This newly-developed advanced DynaHelix Flow technology greatly improve counting precision and accuracy.

DynaScatter Laser

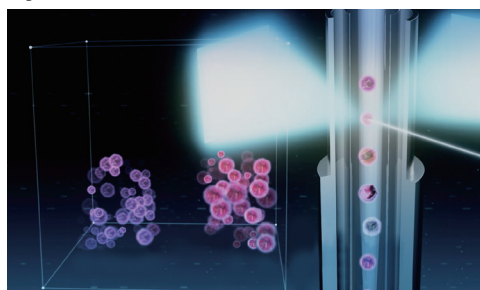

Celltac G's DynaScatter Laser optical technology truly analyzes and differentiates WBCs in near-native state. The innovative 3 angle scatter detector provides better detection of WBCs using precise light scattering measurement. We obtain WBC size information from a small forward angle (FSS), information of cell structure and complexity of nucleo-chromatin particles from a large forward angle (FLS), and internal granularity and globularity information from a side angle (SDS). This 3D graphic information is calculated by the exclusive Nihon Kohden software algorithm.



Solutions simplifying your daily work

Walk Away System



Celltac G's fully-automated random access walk away loading system enables up to 90 tests per hour by just continuously inserting the color-coded racks on the system.

Seamless Information Transfer



Celltac G's HL7 based information system enables seamless bi-directional information transfer to laboratory information systems.



Celltac G reports 33 parameters at once in 40 seconds just with 40μL of whole blood. Newly-added RDWI and Mentzer Index provide clinically-valuable information for differentiating B-thalassemia trait possibility or iron deficiency anemia possibility in microcytic anemia cases.



Also both P-LCR and P-LCC parameters provide information for possible giant platelet, platelet aggregation, or fragment cell presence. These new parameters help faster clinical decision making as well as more accurate diagnosis.



Quality first

Reagent Management



Celltac G's reagent management system helps easier reagent bottle management. With this feature, testing quality is always maintained at high standard level.



Celltac G provides complete traceable QC records that meet laboratory accreditation requirements. In addition, reagent management report, maintenance report, calibration history report, analyzer's daily self-check report and many other reports or logs are always stored using internal memory for evidence of compliance for laboratory accreditation requirements.