

**Product Data****DIAGNOSTIC MAMMOGRAPHY SYSTEM**

# Senoguard-750

**APPLICATION**

The newest technology is melt in Senoguard-750, premium mammography system. It is specially designed for your practice, offers full range of applications and supplies lots of satisfaction as well.

**FEATURES**

- The X-ray high-voltage generator that is equipped with a high frequency inverter system, provides high output and the beam quality best.
  - Magnification radiography (1.5X, 1.8X) employs a micro focus X-ray tube, increasing diagnostic accuracy.
  - The Automatic Exposure Control (AEC) system ensures mammography with stable film density.
    - ✓ The thickness and density of the compressed breast are detected, and the optimal radiography tube voltage is automatically set.
    - ✓ An AEC sensor position can be set. This allows the optimal AEC sensor position to be set according to the projection direction.
    - ✓ The AEC sensor size can be switched between large and small according to breast size. In particular, this function ensures stable AEC radiography for small breasts.
    - ✓ It is possible to automatically set the AEC sensor position according to the C-Arm rotation angle (projection direction).
  - User friendly multiple operation panels improve working condition more efficiently by both side operation.
  - A molybdenum filter (0.03mm Mo) and a Aluminum filter (0.5mm Al) are provided to absorb unnecessary soft X-rays. And a rhodium filter (0.025mm Rh) can be installed as an option (instead of Al filter)
- ✓ Mo filter covers low level kV range (22~35kV) and Al filter covers high kV range (35~39kV) and Mo filter is useful for increasing image contrast in large breast with large amounts of glandular tissue.
  - Both motorized and manual breast compression are available.
  - The supporting C-Arm, with motorized vertical travel of 800mm, is designed for complete axial rotation (+180°/-180°), which makes Senoguard-750 a fully versatile system.
  - ASP (Auto Standard Exposure Positioning) makes your easiest operation and to maximize convenience of Radiography. User can easily set the condition of positioning and exposure with ASP and ASE(CC, RMLO, LMLO). Senoguard-750 C-Arm automatically by one – touch operation for MedioLateral Oblique view and CranioCaudal view.
  - Smart Auto collimation
- Full automatic collimation makes easy



- ✓ Mo filter covers low level kV range (22~35kV) and Al filter covers high kV range (35~39kV) and Mo filter is useful for increasing image contrast in large breast with large amounts of glandular tissue.

- Both motorized and manual breast compression are available.
- The supporting C-Arm, with motorized vertical travel of 800mm, is designed for complete axial rotation (+180°/-180°), which makes Senoguard-750 a fully versatile system.
- ASP (Auto Standard Exposure Positioning) makes your easiest operation and to maximize convenience of Radiography. User can easily set the condition of positioning and exposure with ASP and ASE(CC, RMLO, LMLO). Senoguard-750 C-Arm automatically by one – touch operation for MedioLateral Oblique view and CranioCaudal view.
- Smart Auto collimation

Full automatic collimation makes easy  
(Ver.0809-02)

operation and prevents possible mistakes.

■ Fully motorized ISOcentric C-arm rotation

The center of the image always stays at that same height, which increases efficiency of examination and makes easier positioning for next step.

■ Help menu can make self-diagnosis so that

operators and maintenance representatives will make immediate actions or remote service to the unit. (there are 2 categories with Help codes, codes for users and other codes for technicians

## Composition

### (1) Radiographic table

- ◆ Stand
- ◆ X-ray Tube assembly
- ◆ Stand column assembly

### (2) Generator and Lead Acryl

- ◆ H.V. Generator
- ◆ Controller
- ◆ Lead Acryl

### (3) Standard accessories

- ◆ Compression paddle for 18x24cm

- ◆ Bucky device (18 x 24cm)
- ◆ Spot compression paddle

- ◆ Film marking device
- ◆ Face protection guard
- ◆ A pair of foot switches

### (4) Optional accessories

- ◆ Bucky device for 24 × 30 cm
- ◆ Compression paddle for 24 × 30 cm
- ◆ Magnification device set (1.5X, 1.8X)
- ◆ Hand switch
- ◆ Rhodium (Rh) Filter (Factory option)
- ◆ 2-dimensional biopsy paddle

## TECHNICAL SPECIFICATIONS

### 1-1. Rating

#### (1) Rating at large focus

Tube voltage :	22 to 39KV
Max. tube current :	100mA
mAs :	1 to 600mAs

#### (2) Rating at small focus (for magnification)

Tube voltage :	22 to 35KV
Max. tube current :	30mA
mAs :	1 to 250mAs

### 1-2. H.V. Generator

H.V. generating circuit :	High Frequency Inverter type
High voltage ripple :	less than 1kV
Tube voltage raising time :	less than 2 ms

### 1-3. Controller

Method :	Microprocessor control, Digital display
Radiographic mode :	Manual and AEC mode

### Automatic Exposure Control (AEC)

KV setting range :	22 to 35kV
Max. mAs :	250mAs at small focus 600mAs at large focus

## Product Data of Mammography Senoguard-750

Detector :	Diode
Density :	19 steps
mAs display :	Actual mAs value during AEC radiography is being displayed

Pressure adjustment :	Max. 20 kg (1 kg step)
Radiation field limiting mechanism :	Display of radiation field. The field is illuminated by the light which is lighted by manual switch or by the activation of the down switch by decreasing the compression plate (30sec)

### 1-4. X-ray tube

Type :	Beryllium window, Molybdenum rotating anode tube
Focal points :	0.1mm / 0.3mm
Anode Heat Storage :	300KHU
Target angle :	16 & 10 degree Or 15 degree
Inherent Filtration :	0.63mm Beryllium window

### 1-5. Additional Filter

Kinds of additional filter :	30 $\mu$ m Mo filter and 0.5mm Al filter
Switching method :	Automatic switching by KV setting
Option filter :	0.025mm Rh (32kV-39kV) 30 $\mu$ m Mo (22kV-35kV)

### 1-6. Radiographic table

#### Vertical movement of C-arm

Stroke :	560mm (The distance between 810mm to 1,370mm from floor to radiographic table at 0° position of C-arm)
Lock :	By electromagnetic lock (Off-lock type)

#### Rotation of C-arm

Rotating range:	Right 180° , Left 180°
Lock :	By electromagnetic lock (Off-lock type)
SID :	650mm

#### Compression mechanism

Method :	Manual / Electric
Display of	LED Display
Thickness :	
Pressure plates:	2 kinds

### 1-7. Standard accessories

Bucky device :	- For 18×24 cm cassette size -Grid 4:1, 91line/inch, carbon fiber grid
Compression plate :	2 ea. for 18×24 cm cassette size
Collimator mask :	2 ea.

### 1-8. Optional accessories

Exposure hand switch	
2-dimensional biopsy paddle	1.5 X, 1.8X
Magnification device :	1.5 X, 1.8X
Cassette size :	18×24 cm
Bucky Device and Compression paddle (24 x 30 cm)	
Rh Filter	

### 1-9. Power Supply

Voltage :	Single phase, 200-230Vac , 50/60Hz
Apparent power :	6KVA

### 1-10. Operating condition

Ground	
Ambient temperature :	5 to 40° C
Atmospheric pressure :	70 to 106KPa

## DIMENSIONS AND MASS

Unit	Net					Mass Kg (lb)
	Dimensions (L x W x H)					
	mm (in)					
C-arm stand main unit	1,027	x	692	x	2,066	288
	(40.4	x	27.2	x	81.3)	(636)
X-ray high voltage generator (Control unit)	380	x	600	x	1,752	67
	(15	x	23.6	x	69)	(148)

## INSTALLATION CONDITIONS

### Power requirements

- Single phase AC power supply

Nominal line voltage	200-230 V, 1 $\phi$
Line frequency	50/60 Hz
Allowable voltage fluctuation range (without load)	Within +/-10% of the nominal line voltage shown above
Allowable line impedance	0.36 $\Omega$ or less for 220V
Recommended line capacity	4.5kVA or more

- Maximum line current : 25A at 220V – 10%

### Grounding (3 earthling type)

Grounding must be provided in accordance with all applicable legal requirements for medically used electrical equipment.

### Ambient conditions

- Operating conditions


- ✓ Temperature : 10°C to 40°C
- ✓ Relative humidity : 30% to 50%
- ✓ Atmospheric pressure: 700hPa to 1060hPa

- Transport and storage conditions (while packed)

- ✓ Temperature : -10°C to 40°C
- ✓ Relative humidity : 10% to 90%  
(no condensation)
- ✓ Atmospheric pressure: 700hPa to 1060hPa


Caution: Senoguard-750 must not be used in an explosive gas environment.

**Each assembly**

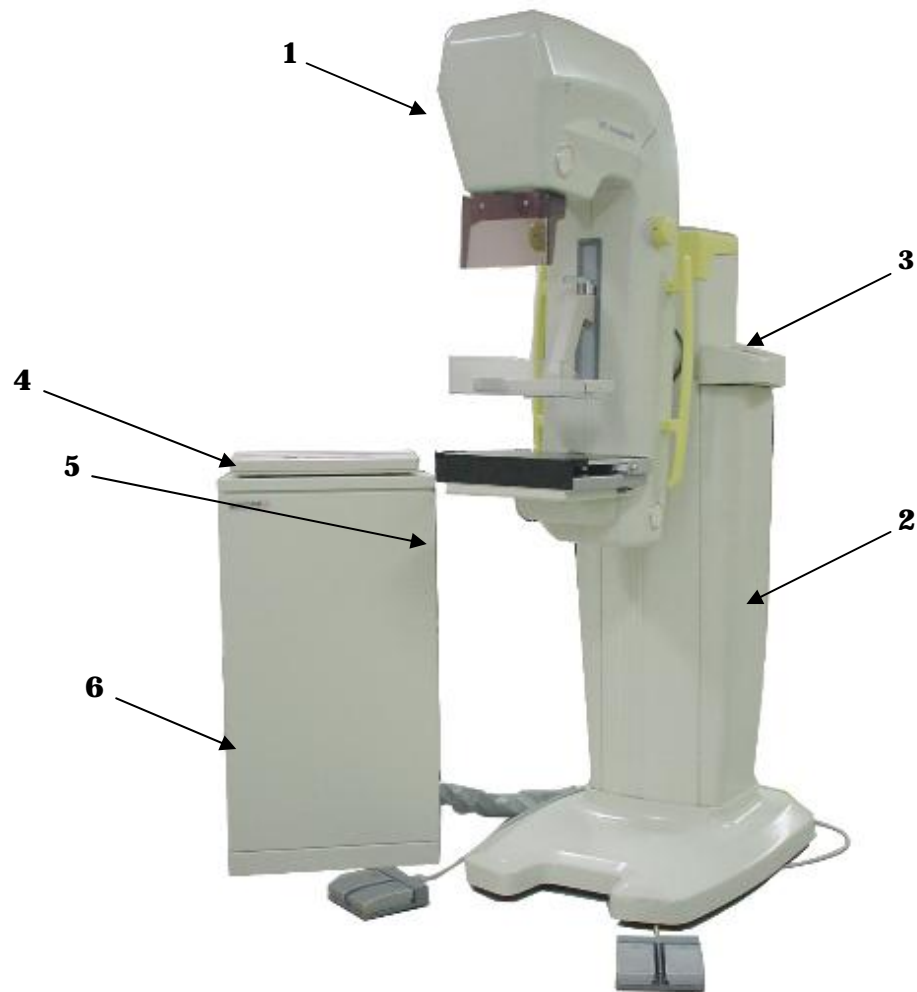


1. C-Arm
2. Stand Column assembly
3. Control panel of Stand column assembly
4. X-ray Control Panel assembly
5. Main Circuit Brake
6. Generator cabinet

## Control Panel

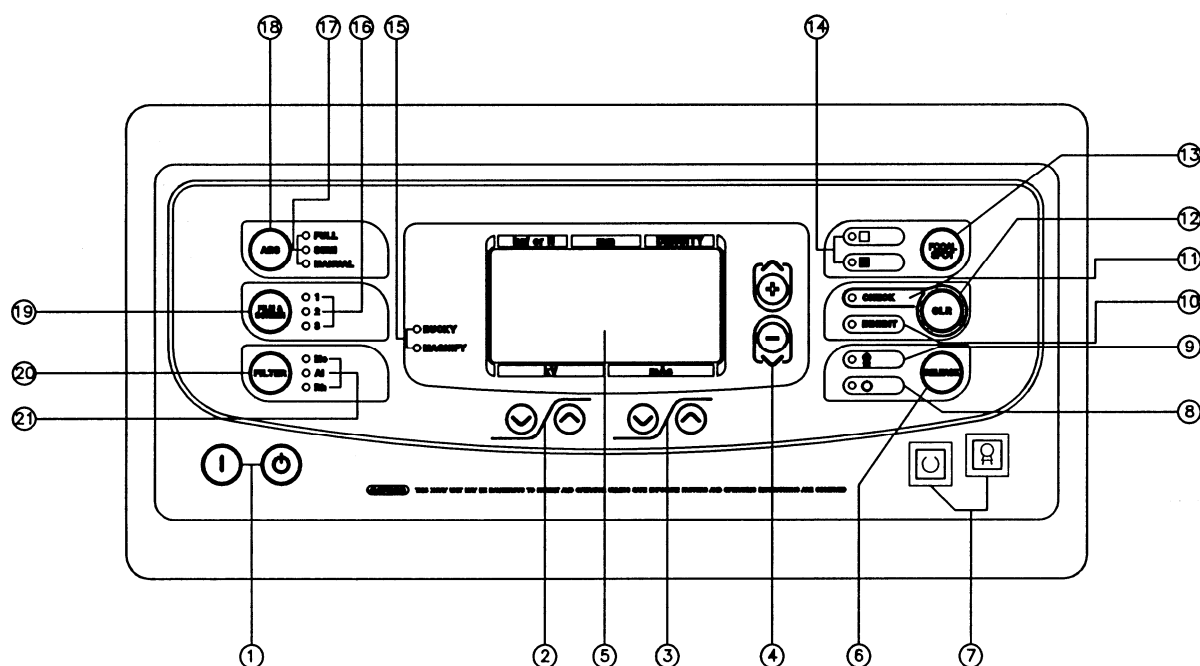

- |                                 |                                   |                                       |
|---------------------------------|-----------------------------------|---------------------------------------|
| 1. Power switch                 | 8. Exposure ready completion lamp | 15. Device check lamp                 |
| 2. kV setting switch            | 9. X-ray exposure lamp            | 16. Film & Screen lamp                |
| 3. mAs setting switch           | 10. INHIBIT lamp                  | 17. AEC selection status indicator    |
| 4. DENSITY setting switch       | 11. Check lamp                    | 18. AEC selection switch              |
| 5. Indicating window            | 12. Clear switch                  | 19. Film & Screen selection switch    |
| 6. Compression releasing switch | 13. Focal Spot switch             | 20. Filter exchange switch            |
| 7. X-Ray ready, exposure switch | 14. Focus status indicator        | 21. Filter selection status indicator |



## Positioning Operation Panel

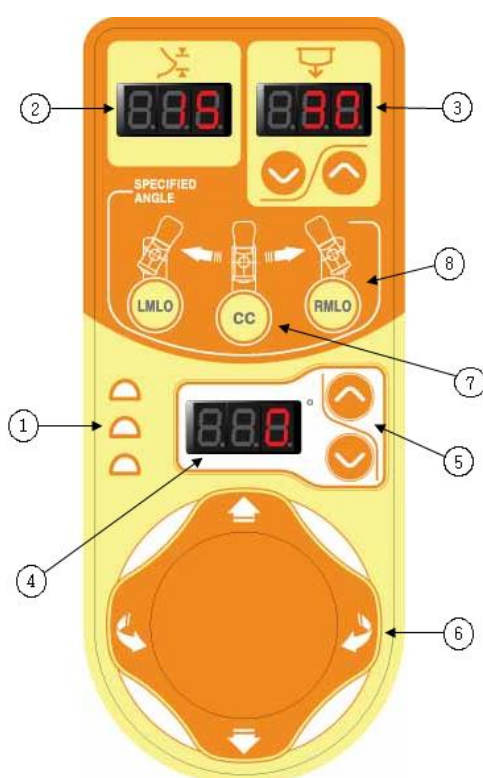

1. Position of Photo timer : AEC sensor position
2. Compression strength displaying area
3. Thickness displaying area (when compressed)
4. C-Arm rotation angle display
5. Rotation stop angle setting switch.
6. C-Arm up/down & rotating button
7. Auto rotation switch (RCC ► LCC )
8. Auto rotation switch (RMLO ► LMLO)

\* ASP means Auto Standard Exposure Positioning which leads to easy positioning for 4 axis standard exposure for a patient. It improves accuracy of positioning and saves total exposure time per patient.

## Overall Dimensions

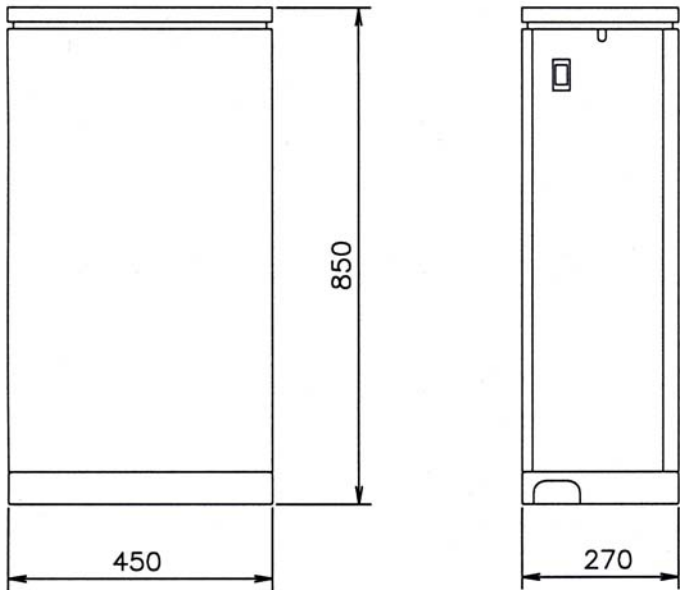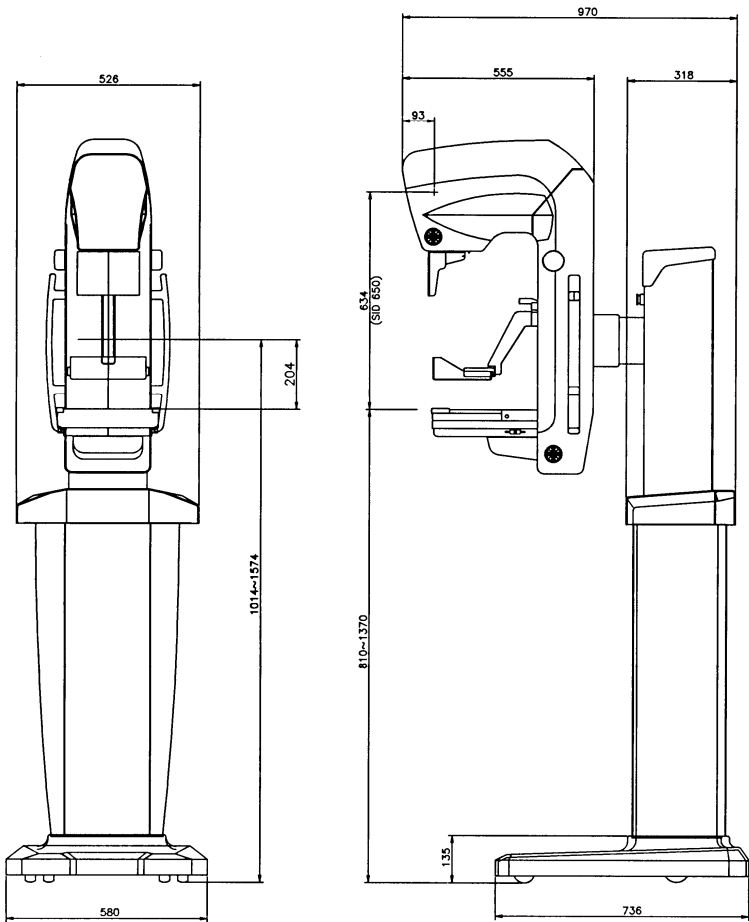

### Compression plate (mm)

- 18 X 24cm standard size (for contact spot exposure)	- 18 X 24cm film size plate (for contact exposure)


### Beam limiting plate (mm)

- Plate for 18 x 24 cm	- Plate for 11 x 12cm (for contact Spot exposure)



### Magnification device (mm)

- 1.5X/1.8X

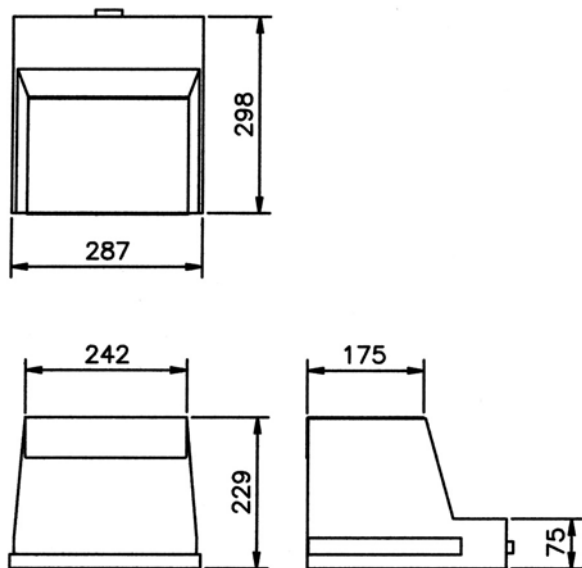


\*Main body weight (355kg)


Part	Weight (Kg)
X-ray tube	10
HV Tank	40
X-ray controller	2
X-ray supporter	278
Protection lead glass	25

### Bucky Device (mm)

- 18 X 24 cm Bucky Device

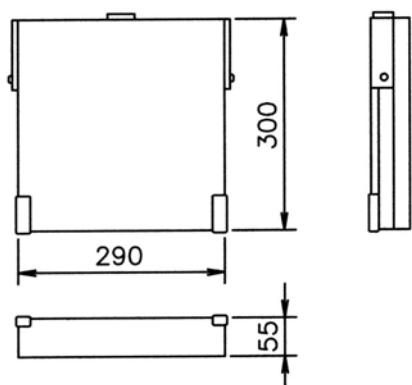

- 24 X 30 cm Bucky Device

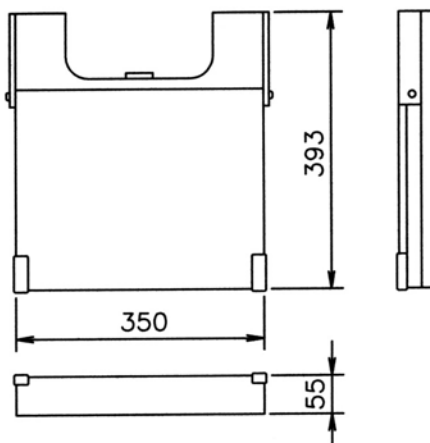

Unsurpassed Image Quality and Easy Operation

**medical ECONET GmbH**

Mainstrasse 6c-d, D-45768, Marl, Germany

TEL)+49 (0)2365 92437-0 FAX)+49 (0)2365 92437-55

EMAIL TO [info@medical-econet.com](mailto:info@medical-econet.com) Visit us at [www.medical-econet.com](http://www.medical-econet.com)